

## P70511

Nomad Biosensors™ comprise a family of genetically encoded fluorescent sensors designed to monitor the signaling of G protein-coupled receptors (GPCRs) in cell-based assays.

Nomad Biosensors™ are engineered to measure the intracellular dynamics of second messengers such as calcium (Ca<sup>2+</sup> Nomad), cAMP (cAMP Nomad), or diacylglycerol (DAG Nomad) upon GPCR activation. Additionally,  $\beta$ -arrestin signaling can also be studied using these biosensors. Nomad Biosensors™ can be combined in the same cell line for multiplex assays.

Prior to GPCR activation, the biosensors are localized in the plasma membrane. Upon ligand binding, the sensors undergo a conformational change that leads to an increase in fluorescence intensity and their relocalization within the vesicular trafficking pathways of the cells.



## cAMPNOMAD ADORA2B

### cAMP Assay

**Product Name:** cAMPNomad-ADORA2B cell line

**Reference:** P70511

**Gene Name:** Adenosine A2B Receptor (ADORA2B)

**cDNA Accession Number:** NM\_000676

**Host Cell Line:** U2OS

**Selection Markers:** Geneticin (G418) + Puromycin

**Cell Quantity:** > 3x10<sup>6</sup> cells/vial


**Storage Conditions:** Liquid Nitrogen

### About cAMPNomad-ADORA2B


Nomad cell lines are a reliable system for studying G protein-coupled receptor (GPCR) signaling in living cells.

Optimized for the integration into High Content Screening (HCS) and High Throughput Screening (HTS) workflows, cAMPNomad-ADORA2B cell line stably express red cAMPNomad Biosensor along with the Adenosine A2B Receptor (ADORA2B).

**Control**

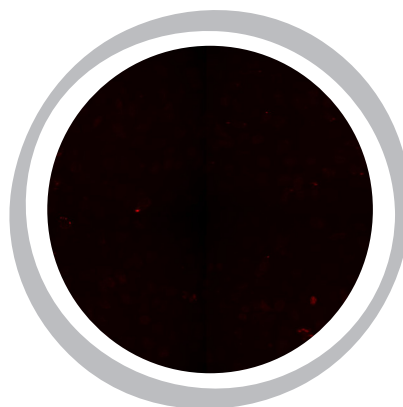

**NECA**

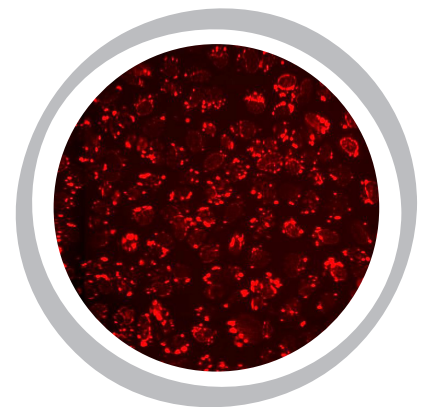


## cAMP Agonism & Antagonism Assays

The  $cAMP$ Nomad-ADORA2B cell line was plated in a 96-well plate and incubated for a minimum of 4 hours and up to 24 hours at 37°C with 5% CO<sub>2</sub> to allow the cells to attach to the plate surface.

**Agonism Assay:** Cells were incubated with NECA diluted in a serum-reduced medium for 20–24 hours.

**Antagonism Assay:** Cells were incubated with PSB-063 diluted in 100 nM NECA serum-reduced medium for 20–24 hours.

The increase (Agonism Assay) or decrease (Antagonism Assay) in the fluorescence intensity of the red  $cAMP$ Nomad biosensor (% Activity) was detected and analyzed using a microplate reader.

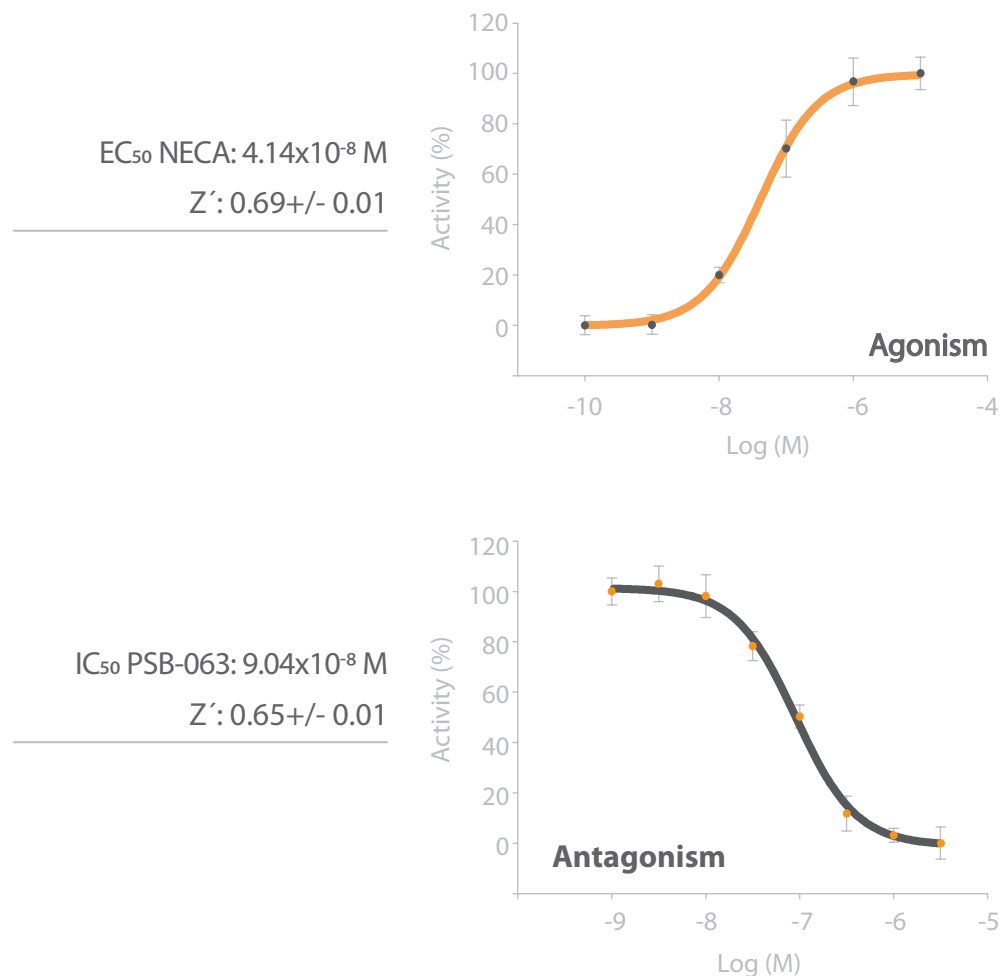

**Figure 1. Dose-response curves for ADORA2B ligands.**

**Top:** concentration response curve for NECA in the agonism assay.

**Bottom:** concentration response curve for PSB-063 for the antagonism assay.

The % Activity corresponds to the fluorescence intensity emitted by the red  $cAMP$ Nomad biosensor normalized against the controls.